


## Quality Passport

### Colloidal solution of silver


Batch number Ag/W 2500 01031  
 General composition of the product silver / medical distilled water  
 Manufacturing date Dez.18, 2023

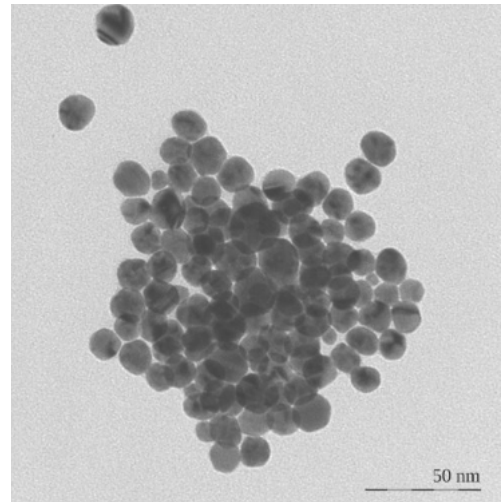

Transmission electron microscopy

### Qualitative indicators

<i>Indicator name</i>	<i>Norm</i>	<i>Analysis result</i>
Appearance	amber-brown liquid	amber-brown liquid
SPR peak, nm	400-420	419
C, Ag/NP mol / liter (ppm)	23.2(2500)	32.2(2900)
pH	7-11	8
Form	Spherical	Spherical
Size	20±5	20±5

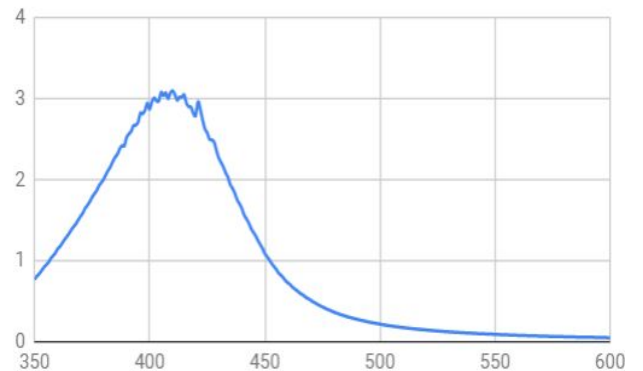

Optical absorbance spectrum

18.12.2023

Technical Laboratory Director

Darin N.I.